

# BPM112: Bidirectional Power Meter for R26 Waveguide

## Contents

General Description .....	1
Specifications .....	2
Pin Assignment .....	3
Nominal Transfer Curves for Analog Outputs .....	4
Typical Directivity .....	4
Typical Linearity Errors .....	5
Sampling .....	6
RS232 Digital Output .....	7
Power Meter Menu .....	7
BPM Monitor .....	9
Dimensional Drawing .....	12
Waveguide Machining Template .....	13
Analog Voltage Outputs Wiring .....	14
Analog Current Outputs Wiring .....	15
Example of BPM Connection .....	16

## General Description

BPM112 is a bidirectional power meter designed for accurate simultaneous measurement of incident and reflected powers up to 30 kW in high-power 2.45 GHz industrial applications using a WR340 (R26) rectangular waveguide. Each power meter is calibrated individually.

The BPM integrates a four-port directional coupler with the following components in each of its two channels:

- Zero-bias Schottky diode detector
- Low noise amplifier
- 16-bit A/D converter for sampling detector voltages
- 12-bit D/A converter providing the analog output
- Microcontroller unit (MCU)
- Optional display (common for both channels)


The MCU:

- Controls both A/D and D/A conversions.
- Performs detector nonlinearity and temperature dependence correction.
- Generates the following simultaneous outputs:
  - Two analog outputs, one (FWD) corresponding to the forward (incident) power; one (RFL) to the reflected power.
  - One digital output (RS232, RS422, or CAN Bus).

The two analog outputs can be

- voltage output 0 – 10 V; or
- current output 4 – 20 mA.

The desired *analog* output type can be switched by the user. Both FWD and RFL outputs are of the same type. The output voltages/currents are linear functions of the microwave powers propagating in the forward and reverse directions of the parent waveguide.

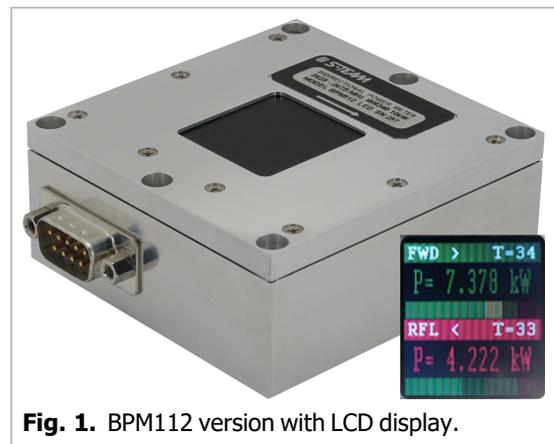

**Fig. 1.** BPM112 version with LCD display.


The digital outputs also provide temperatures of the internal power sensors. The RS232 and RS422 outputs have the form of easily readable text streams. The desired *digital* output type must be specified in the purchase order.

The optional LCD display shows the incident (FWD) and reflected (RFL) powers as well as the temperatures of the internal power sensors. The powers are displayed both numerically and by bar indicators (see the inset in [Fig. 1](#) on the previous page).

BPM is accompanied by the simple Windows-based visualization software **BPM\_Monitor**. LabVIEW instrument drivers are also available.

The BPM module is fastened to a parent waveguide by means of eight M3 or similar-diameter screws after machining of appropriate holes in the waveguide wall.

As an option, one can order a calibrated assembly consisting of a BPM fixed to a precisely machined parent waveguide with the standard length of 174 mm ([Fig. 2](#) above).

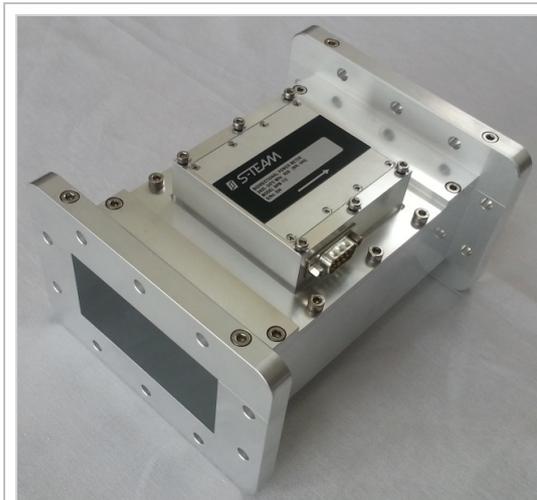

**Fig. 2.** BPM112 (version without LCD display) installed on a standard-length waveguide.

## Specifications


Waveguide of destination	R26 (WR340)
Waveguide wall thickness	2 mm ± 0.025 mm
Waveguide surface flatness required at BPM interface	0.04 mm
Frequency range	2425 – 2475 MHz
Peak working power <sup>1</sup>	0.5 kW, 1 kW, 3 kW, 6 kW, 10 kW, 30 kW
Directivity	25 dB min
Default measurement rate	5 points/s
Max measurement rate <sup>2</sup>	100 points/s
Max sampling duration <sup>3</sup>	5 s
Output voltage polarity	Positive
Power supply voltage	24 V ± 10% DC
Power consumption	4 W / 6 W (without/with LCD display)
Connector	D-sub 9-pin male (D9m)
Dimensions (L x W x H)	80 x 73 x 29.5 mm
Mass (without/with LCD display)	230 g / 300 g
Operating temperature range	-10 °C to +65 °C
Storage temperature range	-20 °C to +80 °C

<sup>1</sup> Peak working power must be specified in the purchase order.

<sup>2</sup> High measurement rates can be attained using high sampling rates and short sampling durations. For details about sampling, please refer to section [Sampling](#).

<sup>3</sup> Sampling duration or integration time is the time over which the samples are acquired for obtaining one measurement data point.

## Pin Assignment

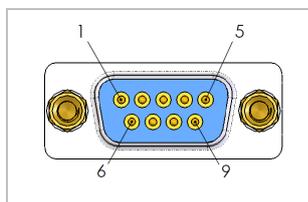


**Fig. 3.** Pin numbering of D9 connector.

Pin	Signal	Description
1	VRFL	Reverse (reflected) power: analog voltage output
2	RX/B-/H	RS232: RX RS422: B- CAN: L
3	TX/A+/L	RS232: TX RS422: A+ CAN: H
4	IFWD	Forward (incident) power: analog current output
5	GND	Signal ground. Negative DC power supply input (0 V)
6	VFWD	Forward (incident) power: analog voltage output
7	IRFL	Reverse (reflected) power: analog current output
8	SHLD	Shielding, Mass
9	VPOS	Positive DC power supply input (+24 V)

### Notes:


- All outputs are referred to GND.
- GND (pin 5) is isolated from SHLD (pin 8).
- The forward wave should propagate in the direction of the arrow on the nameplate.
- Although the pins for the analog voltage output and the analog current output are separate, only one output type at a time can be active.

## Nominal Transfer Curves for Analog Outputs

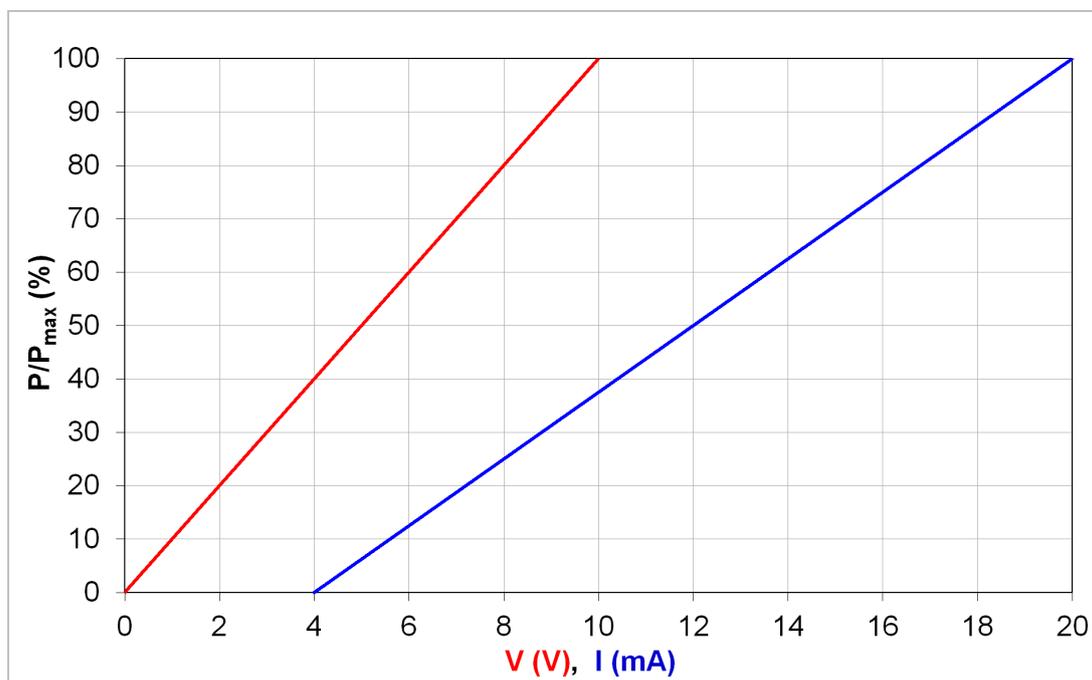


**Fig. 4.** Nominal transfer curves for analog outputs 0 – 10 V, 4 – 20 mA.  $P_{max}$  is the specified maximum working power.

## Typical Directivity

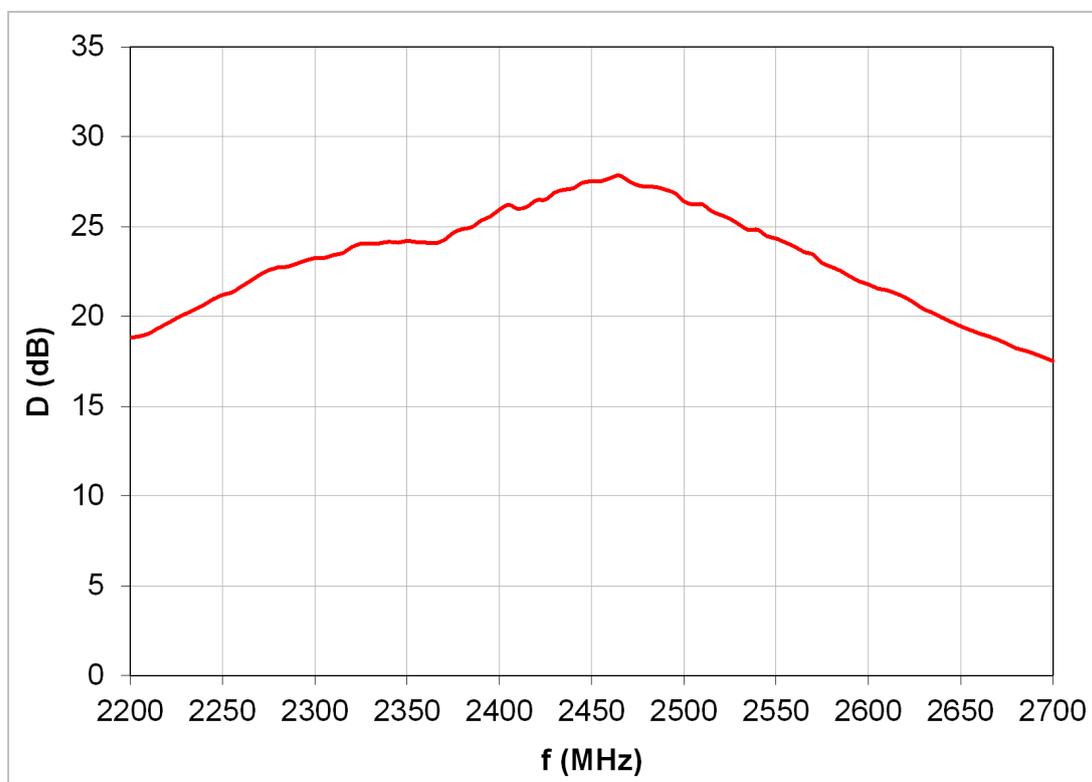


**Fig. 5.** Typical BPM112 directivity (both directions).

## Typical Linearity Errors

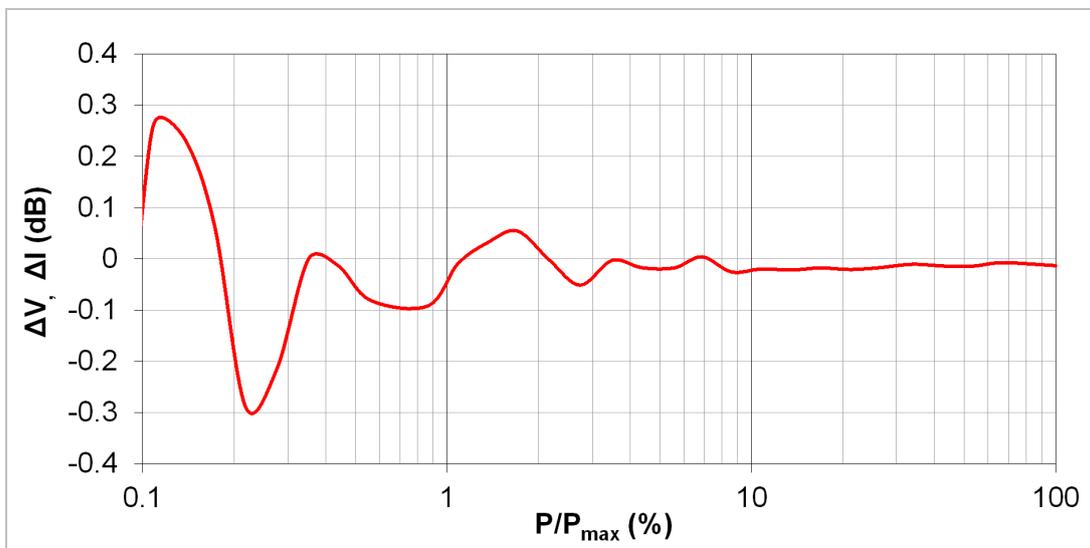

**Fig. 6.** Typical linearity error for analog outputs 0 – 10 V, 4 – 20 mA.  $P_{max}$  is the specified maximum working power.

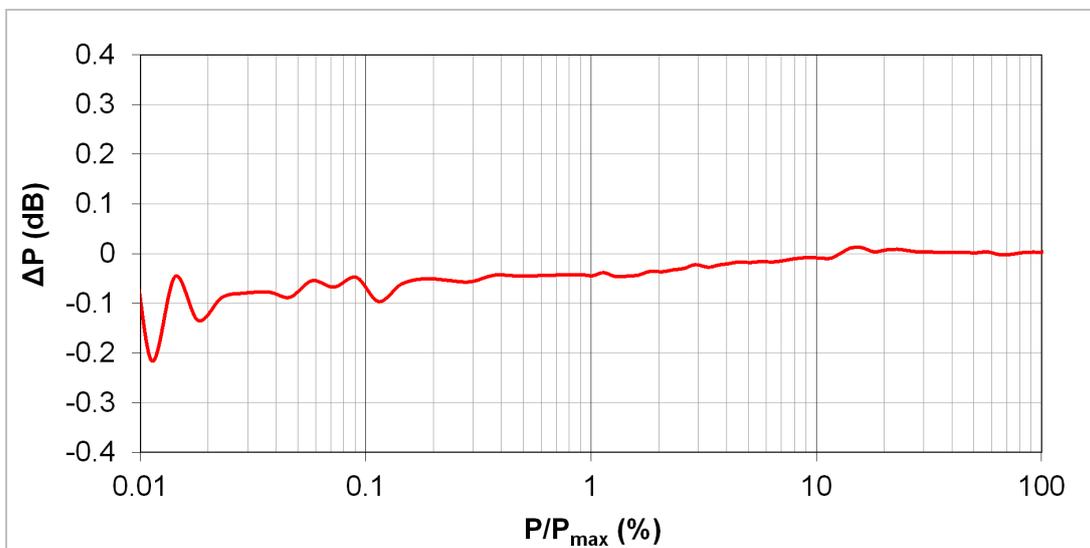

**Fig. 7.** Typical linearity error for digital outputs.  $P_{max}$  is the specified maximum working power.

## Sampling

Both analog and digital outputs are obtained as a result of averaging over a number  $N_s$  of signal samples taken with a specific *sampling rate*  $f_s$  over a specified *sampling time*  $T_s$  (sampling duration, integration time). These sampling-governing quantities are constrained by the relation

$$T_s = \frac{1}{f_s} (N_s - 1) = \Delta t_s (N_s - 1)$$

where  $\Delta t_s = 1/f_s$  is the *sampling repetition period* (time distance between two consecutive samples). The user controls the sampling by defining  $\Delta t_s$  and  $N_s$ ; the resulting sampling duration  $T_s$  is then computed using the above equation.

The values of  $\Delta t_s$  and  $N_s$  can be set by either of these two methods:

- Via any RS232 terminal installed in a PC (see section [Power Meter Menu](#))
- Using the **Terminal** window in the auxiliary [BPM Monitor](#) application

The sampling repetition period  $\Delta t_s$  can be varied in the range 12  $\mu$ s to 10 ms with 1  $\mu$ s step.

The sample count  $N_s$  is defined indirectly in terms of the *averaging exponent*  $E_s$  where  $N_s = 2^{E_s}$ . The exponent can assume the values  $E_s = 0, 1, 2, \dots, 11$ . Consequently,  $N_s = 1, 2, 4, \dots, 2048$ .

To prevent activation of the built-in watchdog (which occurs after 8 seconds of master MCU inactivity), the maximum allowable integration time  $T_s$  is 5 seconds. The user is automatically prevented from entering values of  $\Delta t_s$  and  $N_s$  that would result in a higher  $T_s$ .

**Sampling Rules.** If the signal level is not steady but fluctuates (e.g. due to ripples in the magnetron power supply voltage and/or periodically varying load), two rules in choosing  $\Delta t_s$  and  $N_s$  should be adhered to for accurate and stable mean power display:

1. If the slowest oscillations (ripples) observed in the signal have period  $T_{r\max}$ , the sampling duration  $T_s$  should be equal to an integral multiple of  $T_{r\max}$ , i.e.

$$T_s = n T_{r\max}, \quad n = 1, 2, \dots$$

Alternatively,  $T_s$  can be chosen much longer (at least ten times longer) than  $T_{r\max}$ :

$$T_s \geq 10 T_{r\max}$$

2. The sampling rate  $f_s$  should be at least ten times higher than the *highest* ripple frequency observed in the signal. The minimum sampling repetition period is 12  $\mu$ s (the maximum sampling rate 83 kHz), which enables sampling of amplitude- or pulse-modulated signals with modulation frequencies up to about 10 kHz.

If the signal level is nearly constant (CW, low-ripple), any sampling settings will theoretically work. However, in order to reduce noise and interference,  $N_s$  and  $T_s$  should not be needlessly low. The default settings below are a good compromise.

**Default Settings.** The default sampling repetition period is  $\Delta t_s = 100 \mu$ s. This corresponds to the sampling rate  $f_s = 1$  kHz, which ensures correct sampling of signals with ripple frequencies up to about 100 Hz. The default averaging exponent is  $E_s = 11$ , hence  $N_s = 2048$ . These default settings result in the integration time  $T_s = 204.7$  ms.

**Results Refresh Rate.** Due to the data processing overhead, the maximum cadence of the results production is limited to approximately 100 measurements per second, even when sampling with the highest rate  $f_s$  and the lowest sample count  $N_s$ .

## RS232 Digital Output

After switching on the power supply, BPM starts automatically transmitting data in the form of ASCII strings. The COM port default settings are:

- 8 data bits
- 1 stop bit
- No parity
- Baud Rate 115000 bits/s

The baud rate can be set by the user to 115200, 57600 and 38400 bits/s via the [Power Meter Menu](#).

When connecting a Power Meter with a PLC, please be aware that TX and RX signal leads must be crossed. An example of connecting BPM with a PLC is shown [later in this document](#).

The transmitted ASCII strings are lines of readable text separated by a Line Feed character <LF> (ASCII #10). Normally, each line has the following form:

```
FWD: P= 8.836kW T=38.0 P= 69.46dBm RFL: P= 1.189kW T=38.0 P= 60.75dBm<LF>
```

The line contains two sections, one (FWD) for the forward wave, the other (RFL) for the reflected wave. Each section consists of items of the form **P=Value+Unit** (for powers in kW and dBm) or **T=Value** (for internal temperature in Celsius). The individual items are separated by a space character (ASCII #32). Spaces *within* an item are irrelevant.

In the case of internal ADC overflow, an additional **OVERRRANGE** item occurs, such as (for overflow in FWD channel)

```
FWD: P=120.000kW T=38.0 P= 80.79dBm OVERRRANGE RFL: P= 1.189kW T=38.0 P= 60.75dBm<LF>
```


To obtain numerical values for further processing, the recipient should capture these lines and parse them accordingly.

## COM Port Terminal

In order to test and configure BPM using a PC, one should run an RS232 COM Port terminal program. One possibility is using the open-source free terminal emulator [Tera Term](#). This program can be downloaded from the following [link](#).

For an example of complete BPM – PC connection, see section [BPM Monitor](#) below.

An example of RS232 digital outputs is shown in [Fig. 8](#) below.

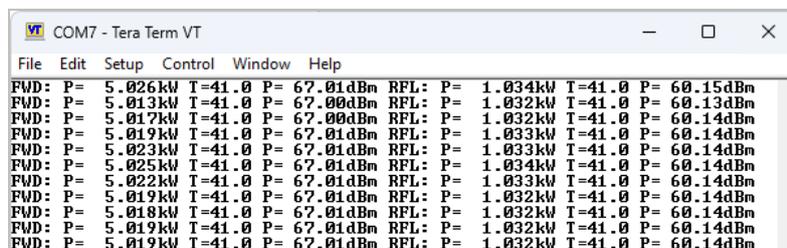

```
COM7 - Tera Term VT
File Edit Setup Control Window Help
FWD: P= 5.026kW T=41.0 P= 67.01dBm RFL: P= 1.034kW T=41.0 P= 60.15dBm
FWD: P= 5.013kW T=41.0 P= 67.00dBm RFL: P= 1.032kW T=41.0 P= 60.13dBm
FWD: P= 5.017kW T=41.0 P= 67.00dBm RFL: P= 1.032kW T=41.0 P= 60.14dBm
FWD: P= 5.019kW T=41.0 P= 67.01dBm RFL: P= 1.033kW T=41.0 P= 60.14dBm
FWD: P= 5.023kW T=41.0 P= 67.01dBm RFL: P= 1.033kW T=41.0 P= 60.14dBm
FWD: P= 5.025kW T=41.0 P= 67.01dBm RFL: P= 1.034kW T=41.0 P= 60.14dBm
FWD: P= 5.022kW T=41.0 P= 67.01dBm RFL: P= 1.033kW T=41.0 P= 60.14dBm
FWD: P= 5.019kW T=41.0 P= 67.01dBm RFL: P= 1.032kW T=41.0 P= 60.14dBm
FWD: P= 5.018kW T=41.0 P= 67.01dBm RFL: P= 1.032kW T=41.0 P= 60.14dBm
FWD: P= 5.019kW T=41.0 P= 67.01dBm RFL: P= 1.032kW T=41.0 P= 60.14dBm
FWD: P= 5.019kW T=41.0 P= 67.01dBm RFL: P= 1.032kW T=41.0 P= 60.14dBm
```

**Fig. 8.** Example of RS232 digital output.

## Power Meter Menu


The Power Meter Menu enables the following operations:

- Configuration of signal sampling.
- Switching the type of analog output.
- Setting the RS232 baud rate.

- Changing the orientation of the LCD display (where applicable).
- Scaling of analog outputs.
- Introducing a power offset to measured data (e.g. to correct for a waveguide wall thickness differing from the nominal).

To use the Menu, an [RS232 terminal](#) must be installed on your PC. The Power Meter Menu is invoked by transmitting either the ASCII character "x" or "X" (ASCII #120 or #88) from the terminal by pressing the **x** or **X** key on the PC keyboard. An example of the BPM Power Meter Menu is shown in [Fig. 9](#) below. For more details, please refer to the application note [AN1601\\_PowerMeterMenu.pdf](#).

As an alternative, one can use the auxiliary [BPM Monitor](#) application.

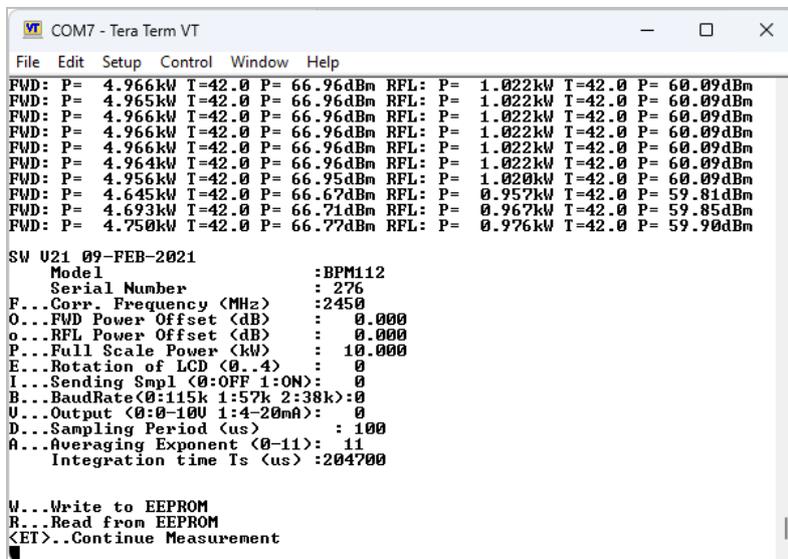

```

COM7 - Tera Term VT
File Edit Setup Control Window Help
FWD: P= 4.966kW T=42.0 P= 66.96dBm RFL: P= 1.022kW T=42.0 P= 60.09dBm
FWD: P= 4.965kW T=42.0 P= 66.96dBm RFL: P= 1.022kW T=42.0 P= 60.09dBm
FWD: P= 4.966kW T=42.0 P= 66.96dBm RFL: P= 1.022kW T=42.0 P= 60.09dBm
FWD: P= 4.966kW T=42.0 P= 66.96dBm RFL: P= 1.022kW T=42.0 P= 60.09dBm
FWD: P= 4.966kW T=42.0 P= 66.96dBm RFL: P= 1.022kW T=42.0 P= 60.09dBm
FWD: P= 4.964kW T=42.0 P= 66.96dBm RFL: P= 1.022kW T=42.0 P= 60.09dBm
FWD: P= 4.956kW T=42.0 P= 66.95dBm RFL: P= 1.020kW T=42.0 P= 60.09dBm
FWD: P= 4.645kW T=42.0 P= 66.67dBm RFL: P= 0.957kW T=42.0 P= 59.81dBm
FWD: P= 4.693kW T=42.0 P= 66.71dBm RFL: P= 0.967kW T=42.0 P= 59.85dBm
FWD: P= 4.750kW T=42.0 P= 66.77dBm RFL: P= 0.976kW T=42.0 P= 59.90dBm

SW U21 09-FEB-2021
  Model          :BPM112
  Serial Number  : 276
F...Corr. Frequency (MHz) :2450
O...FWD Power Offset (dB)  : 0.000
o...RFL Power Offset (dB)  : 0.000
P...Full Scale Power (kW) : 10.000
E...Rotation of LCD (0..4) : 0
I...Sending Smpl (0:OFF 1:ON): 0
B...BaudRate(0:115k 1:57k 2:38k):0
U...Output (0:0-100 1:4-20mA): 0
D...Sampling Period (us)   : 100
A...Averaging Exponent (0-11): 11
   Integration time Is (us) :204700


W...Write to EEPROM
R...Read from EEPROM
<ET>..Continue Measurement

```

**Fig. 9.** BPM Power Meter Menu, model BPM112 shown. Setting E affects only BPM devices with LCD display. Setting F has no effect.

## BPM Monitor


The BPM comes with a simple LabVIEW-based Windows visualization application **BPM\_Monitor**. An example program window is shown in [Fig. 10](#) below.

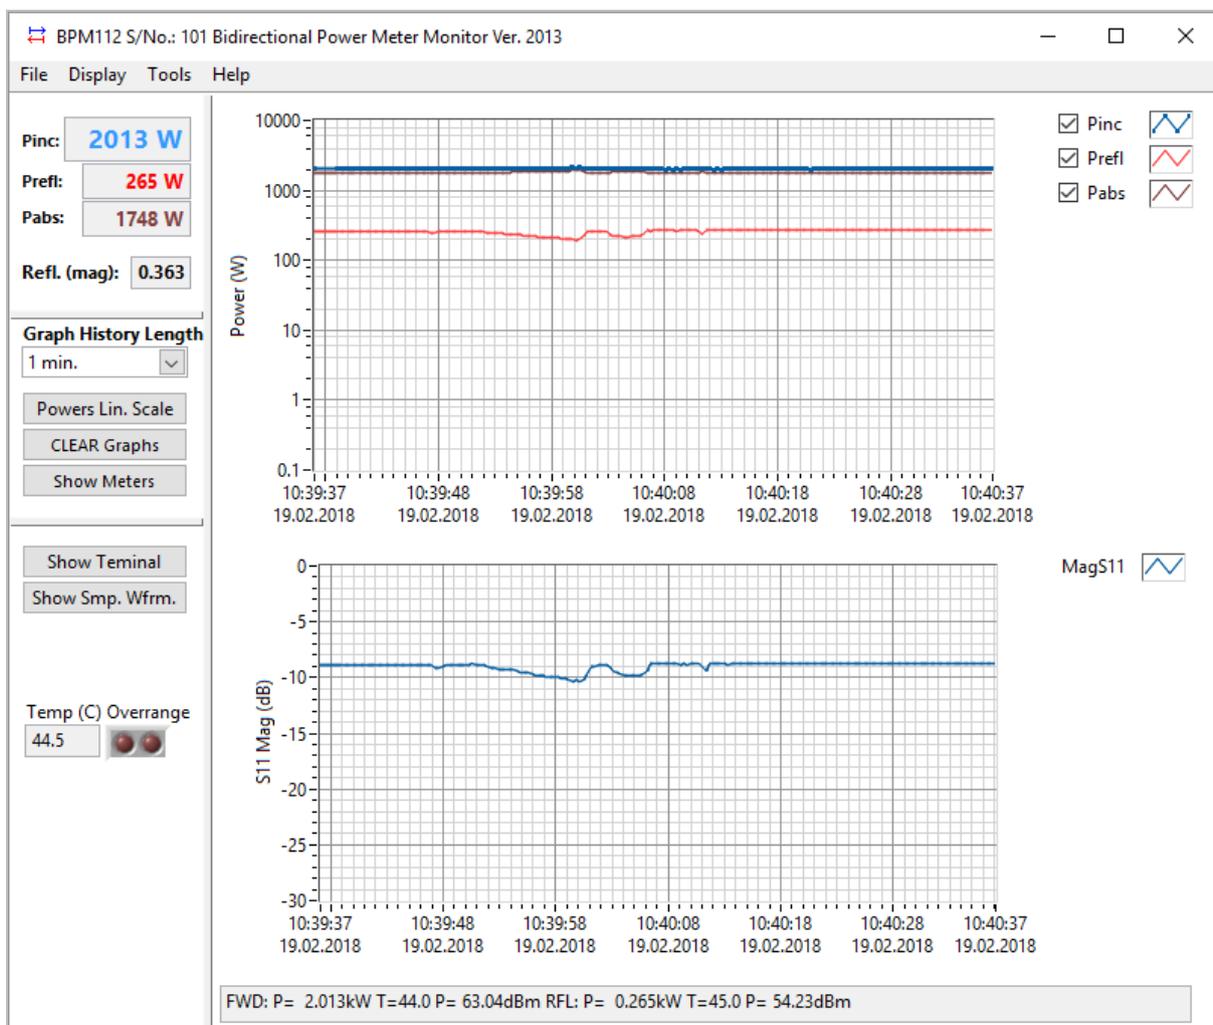

**Fig. 10.** BPM Monitor screen example.


**BPM Monitor** is a program for monitoring and controlling BPM devices. It displays graphs of the incident, reflected and absorbed powers as functions of time. The reflection coefficient magnitude is also displayed in a separate graph. The history of the graphs can be extended to up to 24 hours. All data on graphs can be easily exported to Excel for analysis.

The BPM Monitor also contains a simple RS232 **Terminal** dialog ([Fig. 11](#) on the next page) for setting the internal BPM parameters in a more user-friendly way than by using the [BPM Power Meter Menu](#).

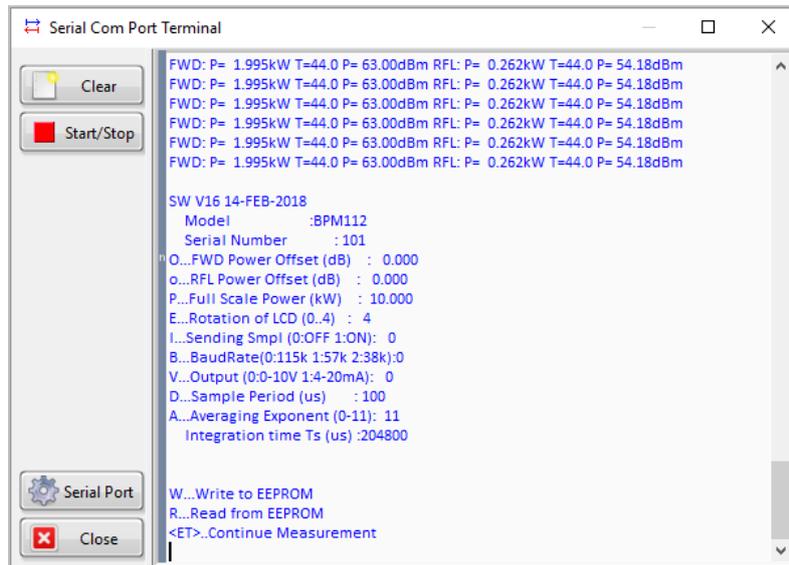

**Fig. 11.** Serial COM Port Terminal window of the BPM Monitor. The example displays BPM Power Meter Menu.

One can perform a more detailed analysis of the generator output waveform with the help of Samples Waveform and FFT Dialog windows, that show the output power as a function of time and its power spectrum, respectively ([Fig. 12](#) below).

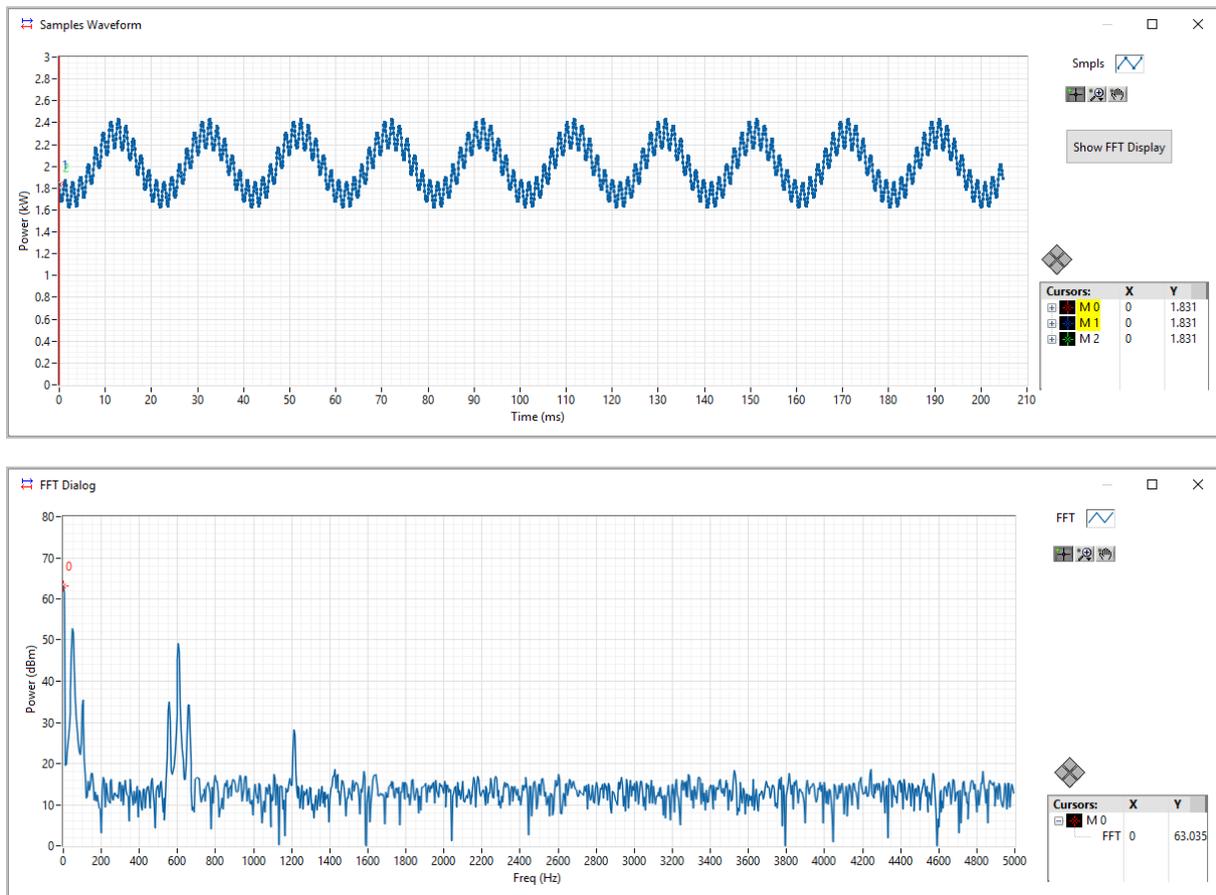

**Fig. 12.** The BPM Samples Waveform and FFT Dialog windows for a twelve-pulse bridge rectifier.

For LabVIEW programmers wishing to develop their own applications, there is a BPM library of virtual instruments available. The library is a part of the BPM Monitor installation package.


If you wish to use the Monitor, please proceed as follows:

- Download the latest installation from <https://s-team.sk/software#bpm> (zipped in a file with a name comparable to **BPM\_MonitorV2031.ZIP**).
- In the case of a zipped installation file, first unpack the zip file.
- Run the installation program (**setup.exe**).
- After installing, connect the BPM to your PC. You will need the following:
  - 24V DC power supply.
  - Extension cable, branching the DC power supply inputs VDC and GND to the power supply and TX, RX, GND pins to standard D9 RS232 connector. You have to make this extension yourself.
  - Standard RS232 cable (a null modem, i.e. a type with crossed RX/TX leads).
  - RS232-to-USB adapter. In case of problems, we recommend the Brainboxes US-101 (supplied worldwide e.g. by Farnell).

An example of the BPM connection with a PC is shown in [Fig. 17](#) on page 16. The same connection applies to the [COM Port Terminal](#) emulator.


- On the PC, run **BPM\_Monitor.exe** (shortcut  found on the PC desktop). In the program, you will be asked to choose an appropriate COM Port. Then the measurement should start.

### Dimensional Drawing

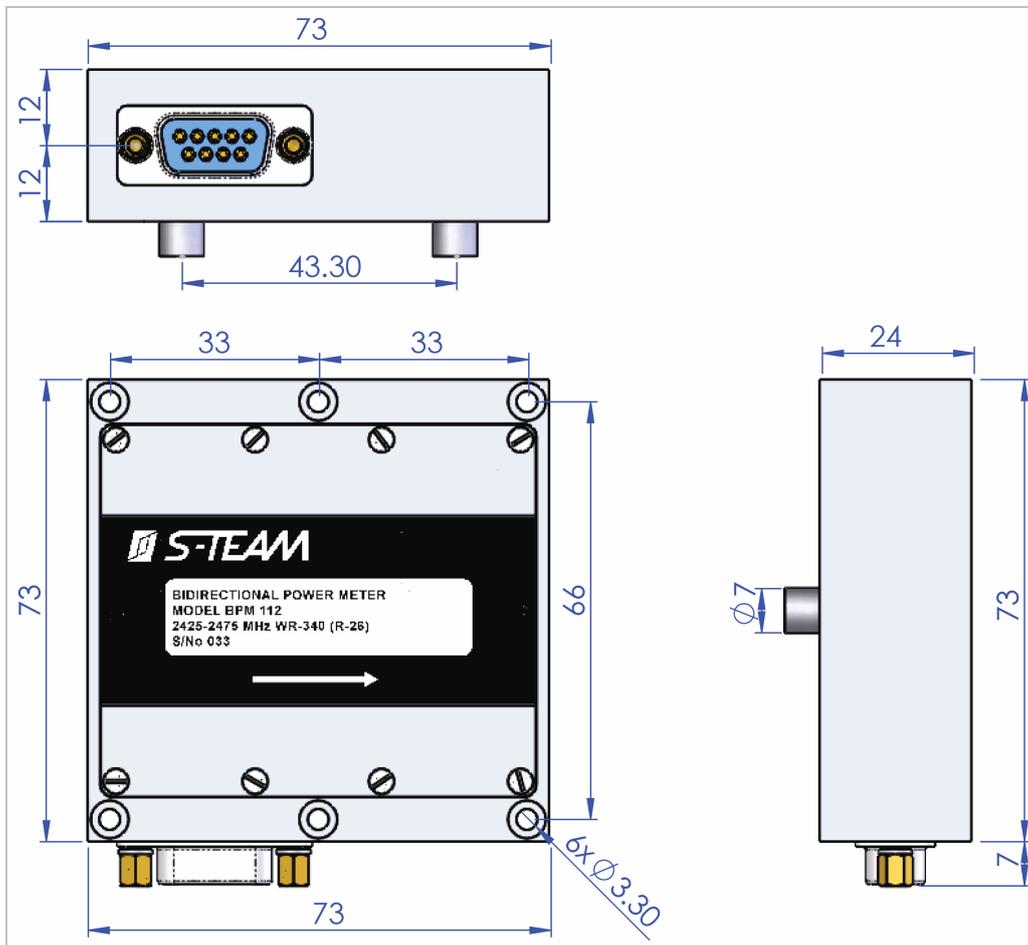

**Fig. 13.** Basic BPM112 dimensions in millimeters. The probe protrusion is 5.5 mm.

## Waveguide Machining Template

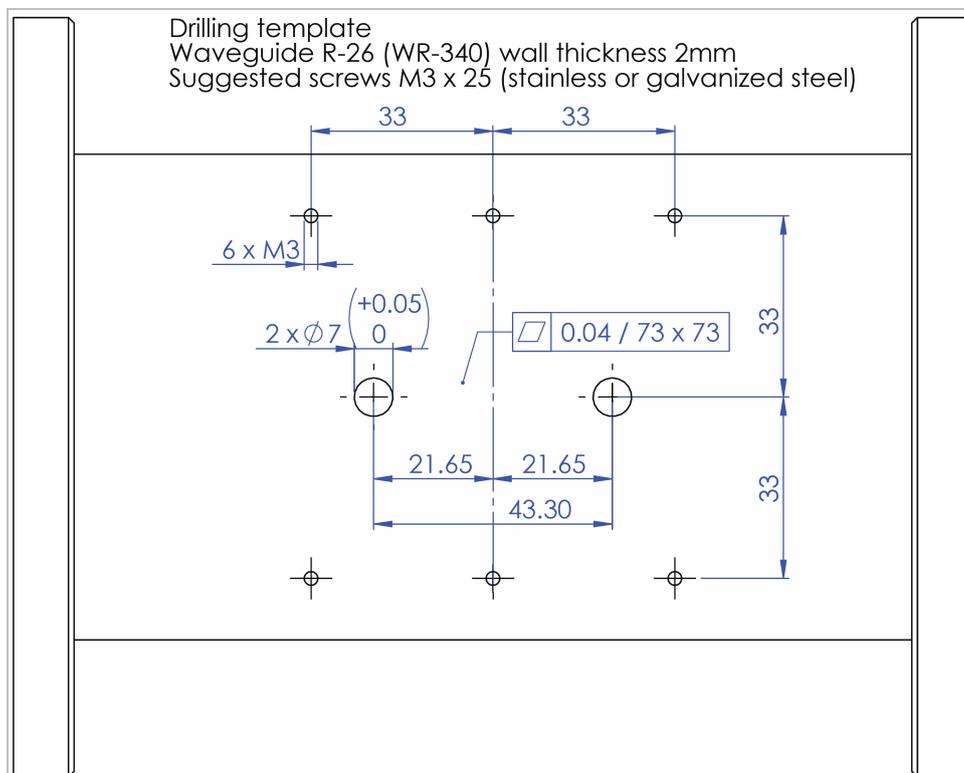

**Fig. 14.** Waveguide machining template. All dimensions are in millimeters. The pattern is centered about the waveguide axis. The waveguide wall thickness must be 2 mm.


### Important Note

Complying with the specified waveguide wall thickness and flatness of its surface interfacing with the BPM is essential in order to achieve the specified measurement accuracy. The slope of the coupling factor as a function of the wall thickness is about -6 dB/mm (i.e., increasing the wall thickness decreases the output power readings).

If the wall thickness differs from the specified figure but is known, one can apply a user-defined correction based on the above slope. Nevertheless, the wall thickness should not deviate from the specification by more than  $\pm 0.3$  mm, otherwise BPM directivity will deteriorate.


To avoid problems with manufacturing precision waveguide components, one can order a calibrated assembly consisting of a BPM module fixed to a parent waveguide. The standard waveguide length is 174 mm.

## Analog Voltage Outputs Wiring

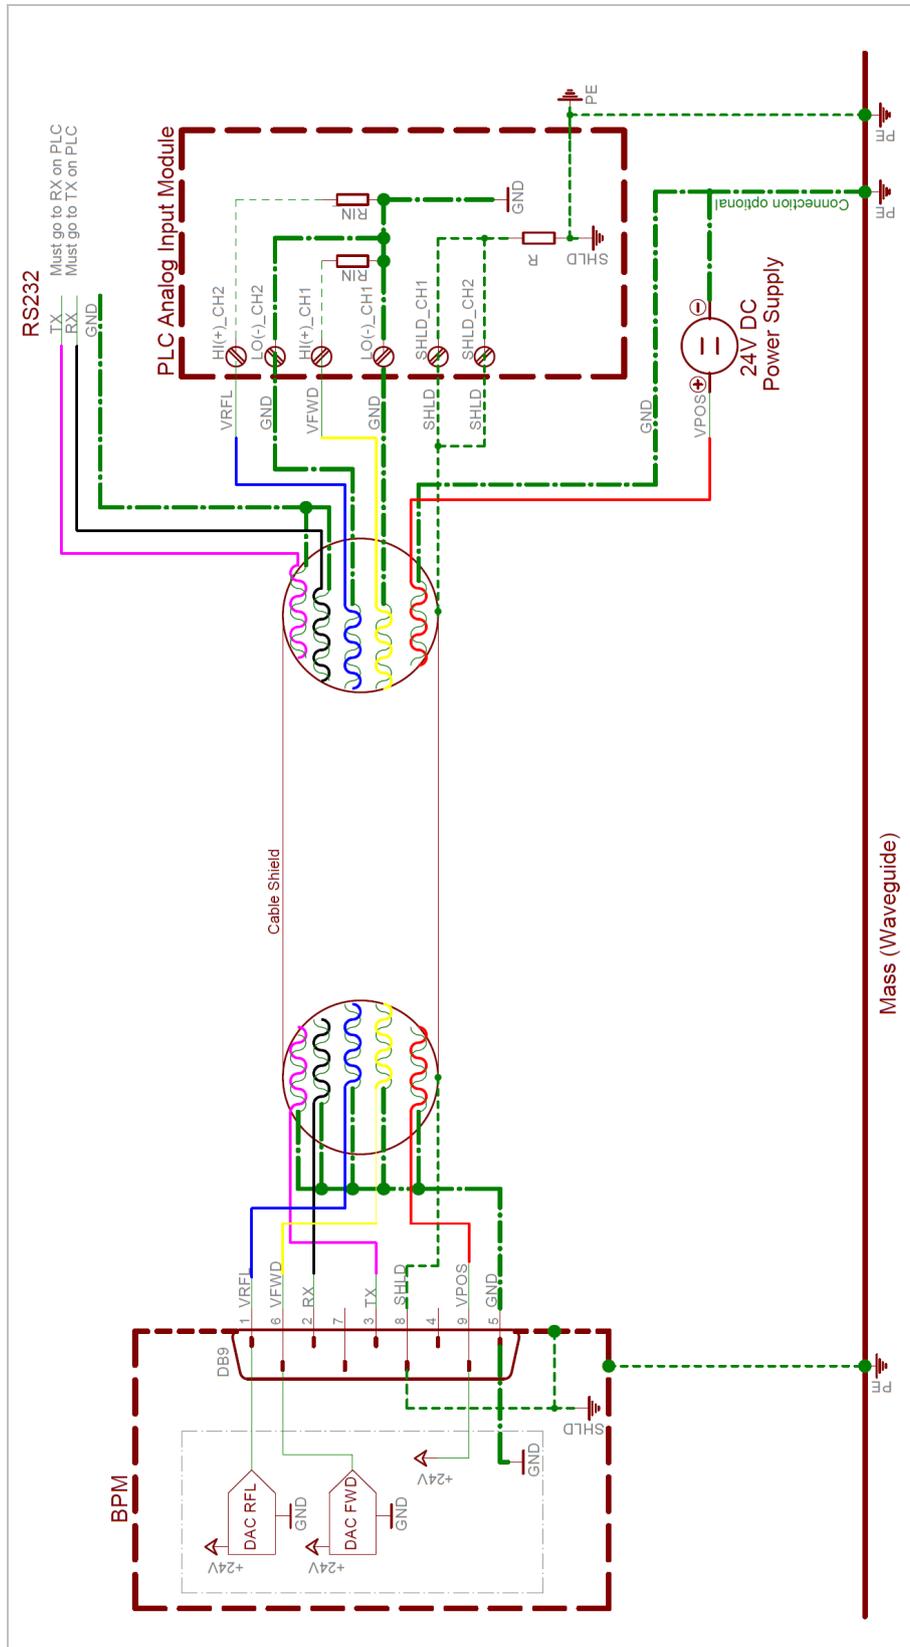

**Fig. 15.** Example of BPM – PLC wiring for analog voltage outputs.

## Analog Current Outputs Wiring

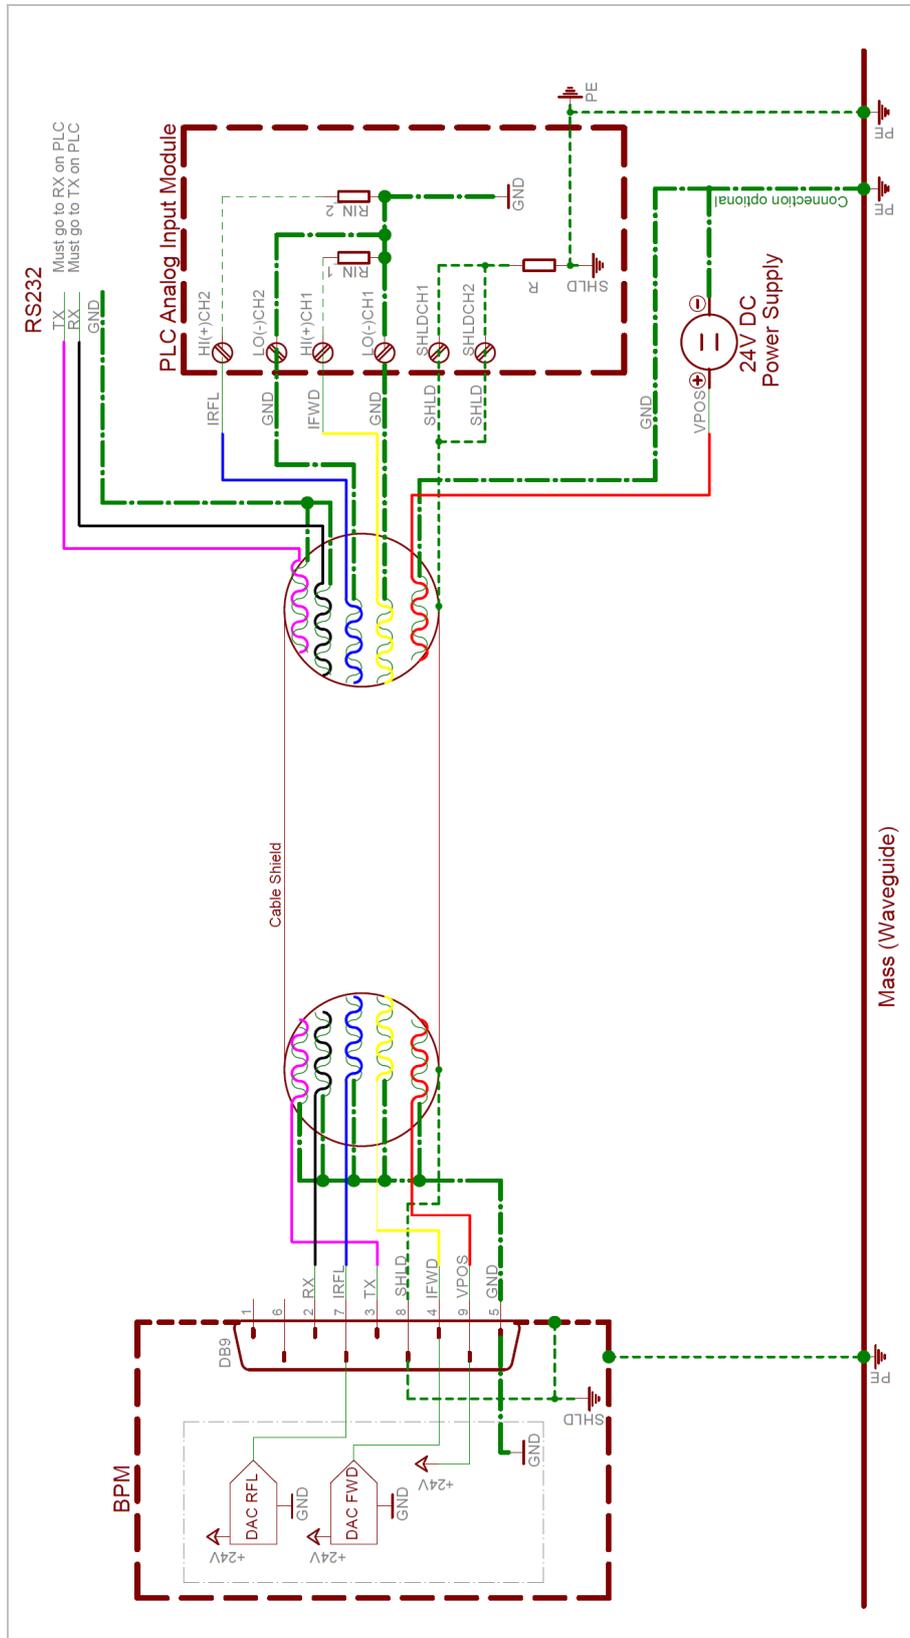

**Fig. 16.** Example of BPM – PLC wiring for analog current outputs.

## Example of BPM Connection



**Fig. 17.** Illustration of BPM – PC connection.